

QUICK START GUIDE

How to Set your IRwin Methane Leak Detector for 1 Point Calibration
2.2% (2.5%) - Universal Mode
(for a factory set unit)

1

Make sure your IRwin is set in Universal Mode (see the *How to set your IRwin for Universal Mode* quick start guide)

2

Press  followed by 

3

Use  to navigate to *General* and press 



4

Use  to navigate to *Custom* and press 



5

Use  to navigate to *AbG Cal Setup* and press 



6

If prompted, enter the Supervisor (Advanced) password code
 If not prompted, go ahead to next step

7

Use  to select *Generic* and press 
 followed by 



8

Use  and  to navigate to *Calibration*
 and press 



9

Use  to navigate to *Settings* and press 




10

If prompted, enter the (min) Intermediate password code
 If not prompted, go ahead to next step

11

Press  to get to the drop-down menu

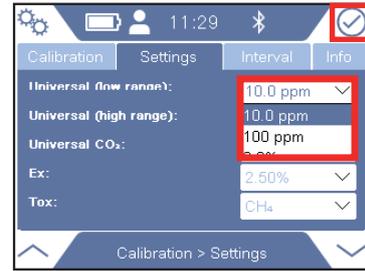

12

Press  on the first choice of the drop-down menu



13

Navigate to far right drop-down menu and press 



14

Use  to select *Disabled* and press 




15

Press  again to view drop-down menu




16

In *Universal Low Range*, use  to select the second choice in the drop-down menu, press 

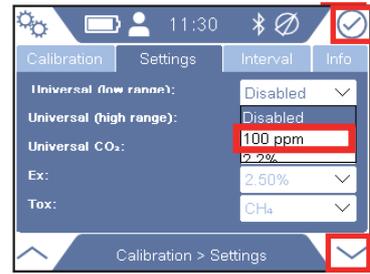

17

Navigate to far right drop-down menu and press 

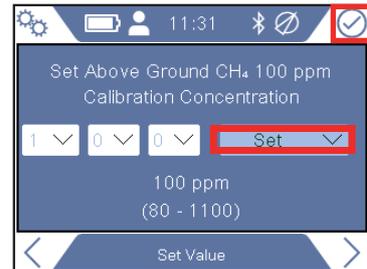

18

Use  to select *Disabled* and press 




19

Press  again to view the drop-down menu



20


In *Universal Low Range*, use  to select the third choice in the drop-down menu, press 

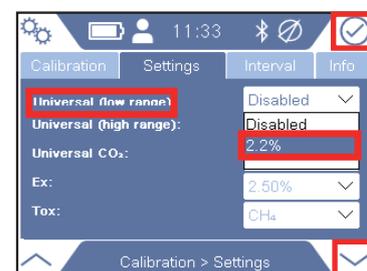

21


Use to navigate to drop-down menus. Set the actual value of the calibration gas you have, nominally 2.2% or 2.5%, by entering:

2 and press
2 (5) and press

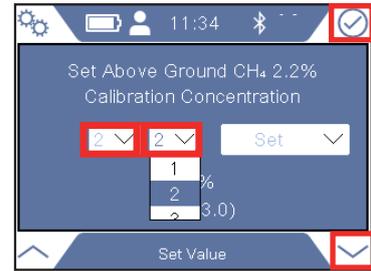

22

Navigate to far right drop-down menu and press

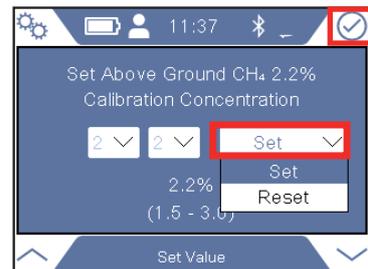

23

Select Set by using and and press



24

Press followed by and